


# Quick Start Guide - Dali care bed

## Safety sides


### Raising

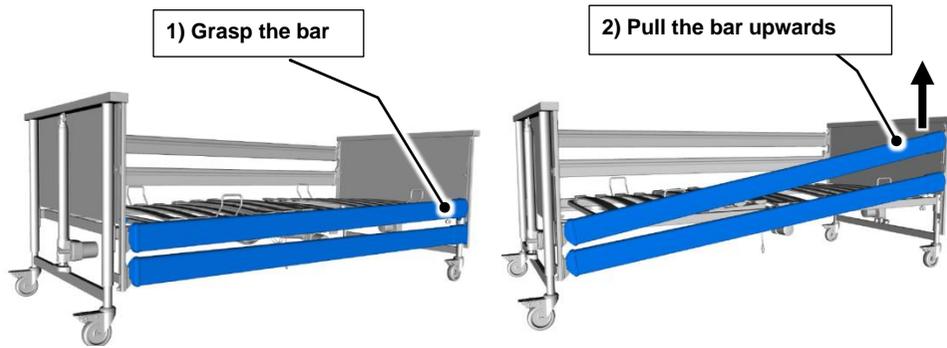

3) Check that the safety side bars are securely locked in place by pressing down on them.

4) Repeat the process on the other side.


### Lowering

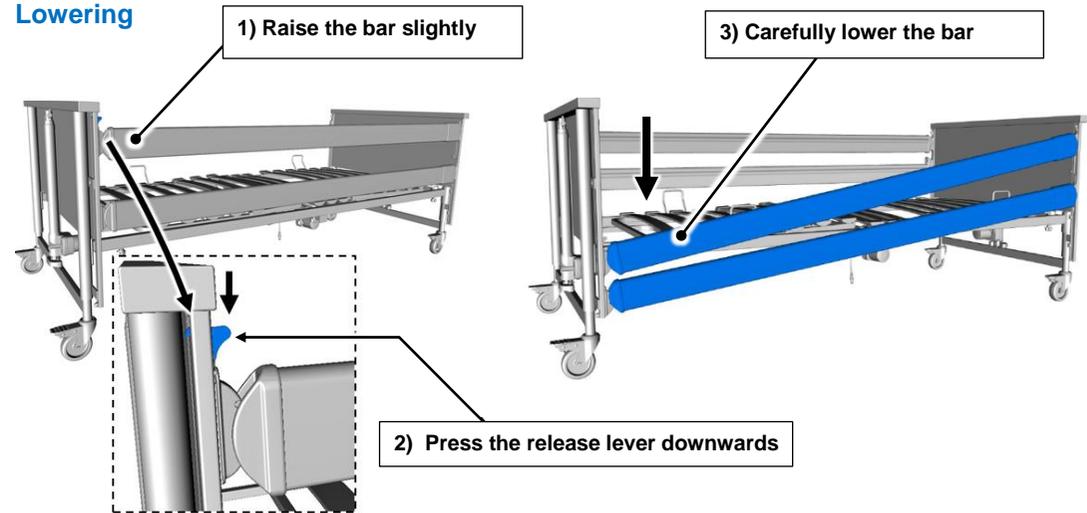


4) Repeat the process on the other side.

## Triangular grab handle

### Adjusting horizontally

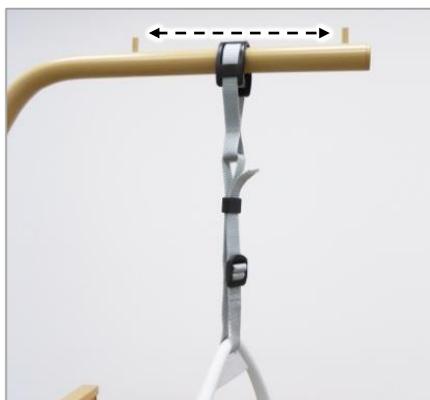

### Adjusting vertically

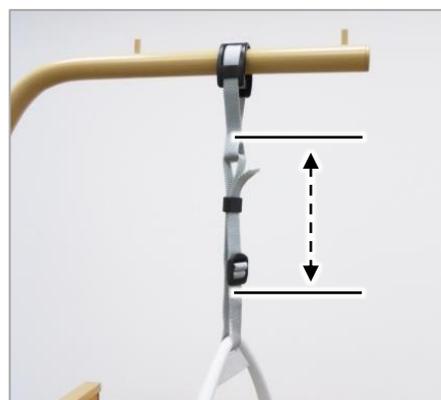

### Operation (shortening/lengthening)


Draw the strap ① through the buckle ② :

**To shorten:** Pull the end of the strap ③ upwards

**To lengthen:** Pull the triangular grab handle ④ downwards

**i** Maximum loading capacity 75 kg.


**i** Make sure when lengthening the strap that the end of the strap projects at least 3 cm beyond the top of the buckle.

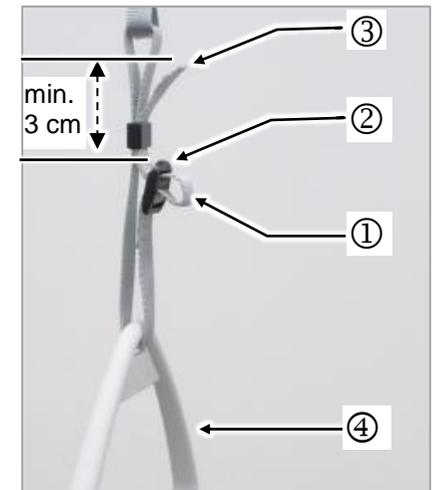


## Bluetooth handset (wireless)

(In the Dali standard, Dali low-entry and Dali wash)

- 1 Backrest
- 2 Mattress base height
- 3 Thigh rest
- 4 Reverse-Trendelenburg position
- 5 Magnetic sensor (identifiable by cross-hair symbol)
- 6 Sleep position
- 7 Battery symbol
- 8 LED
- 9 Locking symbol

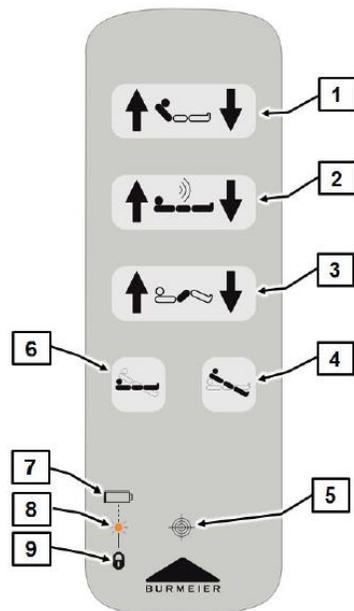

The following basic rule applies:



Explain the handset functions to the resident!

- The electric motors operate as long as the corresponding button is pressed.
- With the exception of the reverse-Trendelenburg position and sleep position, all of the bed's adjustment options work in both directions.
- The handset is water-protected and can be wiped clean with a cloth.
- The handset can be hung on the bed with its elastic hook.

## Locking function – Bluetooth handset


Please note:

There is a magnetic sensor at the bottom of the handset.

A loose magnet **a** (part of the delivery) is required to lock or unlock functions.

Proceed as follows to lock/unlock adjustments on the handset:

- Hold the supplied magnet **a** to the magnetic sensor integrated in the manual switch
- Then lock/unlock the desired function.
  - To lock, press the right button on the handset. To unlock, press the left button (see following table).

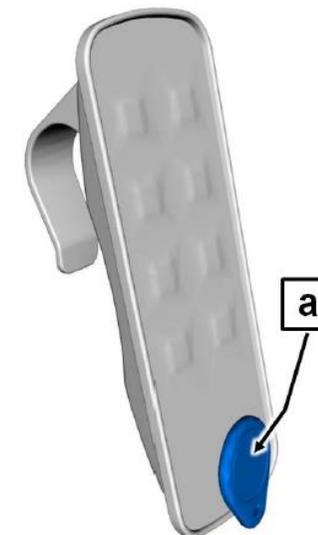

Unlock	Function	Lock
	Backrest	
	Mattress base height	
	Thigh rest	
	Sleep position/reverse-Trendelenburg position	

## Coupling the handset with the control unit (only in the Dali standard, wash and low-entry)

 Please note: Before the bed functions can be adjusted, the handset must be coupled (connected) with the control unit.

Coupling is only necessary when commissioning the bed, replacing the Bluetooth handset and replacing the control unit.

Proceed as follows:

1. Plug the power pack into the electric socket.
  - If the power pack was already in the socket, remove the power pack from the socket, wait approx. 10 s and plug it in again.
2. Within 20 s, press the two buttons for up/down mattress base height simultaneously (within 0.5 s) for at least 5 seconds.
  - The LED on the control unit lights up orange for 4 seconds if coupling was successful.
  - The LED on the control unit flashes orange 4 times if the coupling was not successful. In this case, repeat steps 1 and 2.

## Battery – Bluetooth handset

 The Bluetooth handset is powered by a CR 2032 lithium battery.

When the battery is low, the LED display on the handset flashes yellow 4 times each time the button is pressed. The battery must then be replaced within a few days.

Proceed as follows:

1. Open the battery compartment cover  on the back of the handset.
  - For example, insert a coin into the slot of the cover and turn it counter-clockwise.
2. Remove the old battery.
3. Insert the new battery (observe polarity).
4. Close the battery compartment with the cover (turn clockwise).



# Quick Guide - Dali care bed

## Cable handset

(In the Dali standard, Dali low-entry and Dali econ)

### Operation



The following basic rule applies to the keys:

Raise: Lower:

For safety reasons, the handset is equipped with a locking function.

Turn the lock clockwise to the locked position using the locking key.

The colour of the respective display changes from green to yellow.

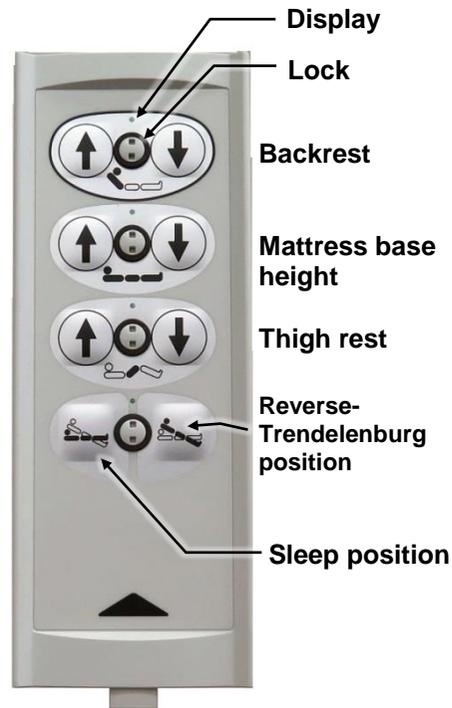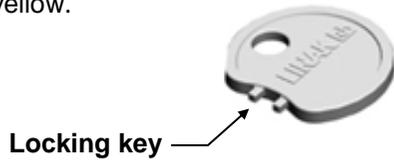

Do not forcibly turn the locking key! The lock or the handset could be damaged.

**Actuator released:**  
The lock is in a vertical position  
Colour of display: green  
Keys can be operated ("click" sound)


**Drive locked:**  
Lock turned approx. 15° clockwise  
Colour of display: yellow  
Keys are locked

## Castors - operation

**Caution!** Operate the castors with the foot only.  
Wear closed shoes when operating the bed to avoid foot injuries.

**Moving:** Raise the pedal with the top of your foot.

**Braking:** Press the pedal down with your foot.

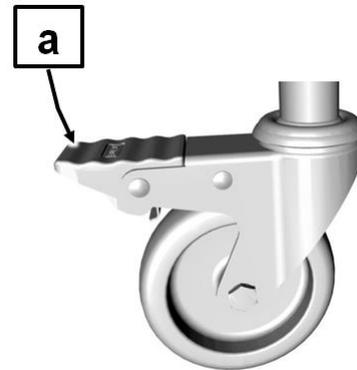

### CAUTION

The Quick Start Guide does not replace the main instruction manual for the Dali care bed.  
Read the main instruction manual carefully and observe the safety instructions!